




BioSmart®

Oxygen Uptake Comparison pH 5.0

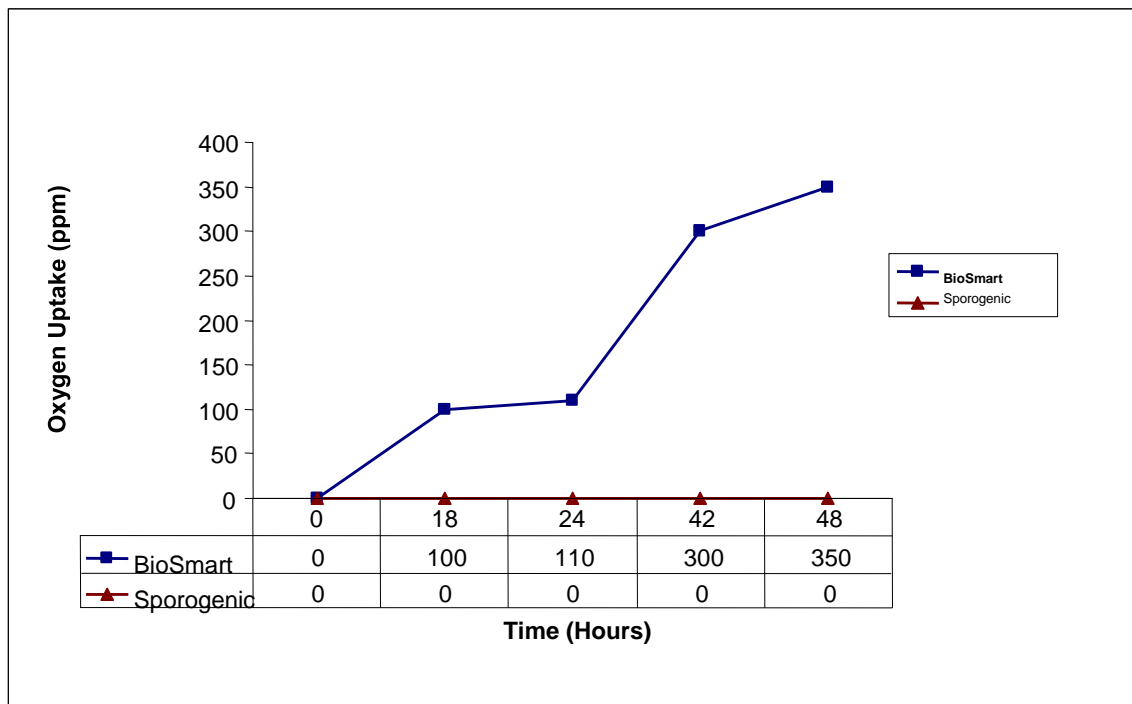

- BioSmart® shows positive activity at pH 5.0
- Sporogenic products are not active at pH 5.0